



KONICA MINOLTA

NEW

SPECTROPHOTOMETER **CM-3700A**

THE NEW LEADER

Konica Minolta's flagship model: High accuracy and repeatability even at low reflectance/transmittance



The essentials of imaging

A high-accuracy, top-class model filled with Konica Ideal for demanding customers with strict requirements

An advanced spectrophotometer for reflectance and transmittance measurements of a broad range

Top-of-the-line model providing high accuracy and high reliability

Konica Minolta's advanced optical, sensing, and signal-processing technology provide excellent repeatability.



Strictly selected high-quality parts ensure long-term stability and reliability.

Strict accuracy control traceable to national standards ensures high quality with high inter-instrument agreement.

- 1 Illumination/viewing geometry conforms to CIE, ISO, ASTM, DIN, and JIS requirements for di:8°, de:8° (diffuse illumination/8° viewing) geometry for reflectance and to CIE, ASTM, DIN, and JIS requirements for transmittance.
- 2 Pulsed xenon arc lamp light source provides high stability, long life, and excellent repeatability even on dark and high-chromaticity colors.
- 3 6-inch integrating sphere has a powdered barium sulfate (BaSO₄) coating with superior optical characteristics.
- 4 Double-beam feedback system directly monitors the light emitted by the xenon lamp at the time of measurement and automatically compensates for changes in brightness or spectral characteristics to ensure high-accuracy measurements.

- 5 Polychromatic unit
A diffraction grating ⑤ provides high-efficiency separation of light by wavelength, ensuring high repeatability even when measuring dark colors, and the silicon photodiode array sensor ⑥ quickly converts the separated light into electrical currents. These elements are mounted on stainless steel with a low coefficient of thermal expansion to ensure long-term stability.
- 6 The optical systems for sample measurement and light-source monitoring are mounted on an aluminum alloy block for long-term stability.

* CM-3700A is computer-controlled.
Software such as optional SpectraMagic™ NX required.

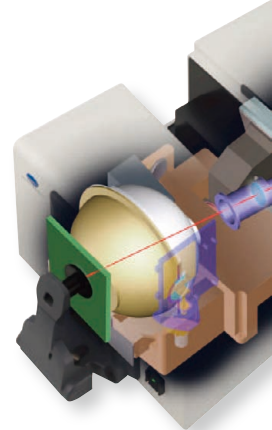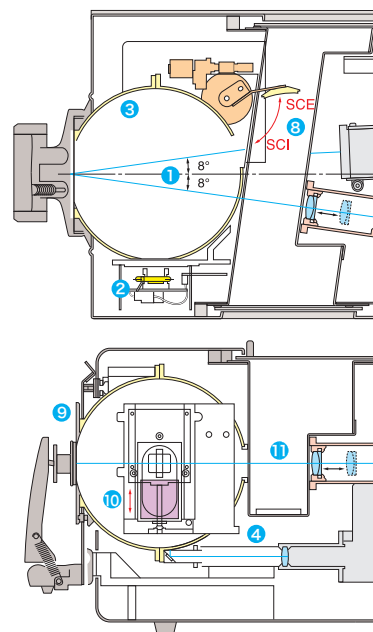

Comprehensive mea

Reflectance measurements

- 8 Switchable between SCI and SCE measurements
SCI (specular component included) measurements minimize the influence of surface conditions on measured values, making it suitable for CCM applications. SCE (specular component excluded) measurements correspond closely to professional visual evaluation.
- 9 Selectable measurement areas
Measurement areas of Ø25.4mm, Ø8mm, and 3×5mm (rectangular) can be selected according to the application.

- 10 Variable UV for measuring fluorescent samples
The UV cut filter can be adjusted in 1000 steps for measurements of samples containing optical whitening agents such as paper, pulp, etc.



Transmittance measurements

- 11 Sideless transmittance chamber
(Maximum thickness: Approx. 50 mm)
di:0°, de:0° (diffuse illumination) spectral transmittance measurements as glass, filters, etc. as well as such as foods, cosmetics, etc.




Konica Minolta's advanced optical technology. Instruments for R&D, QC, and CCM applications.

Full data
compatibility
with CM-
3700d

of subjects including pigments, dyes, plastic, textiles, paints, ceramics, etc.

Top standard instrument for color control systems

With its high accuracy, high repeatability, and high reliability, the CM-3700A can be used as the top standard instrument to which other instruments are referenced in color quality control systems including multiple instruments, both within a company or between companies.

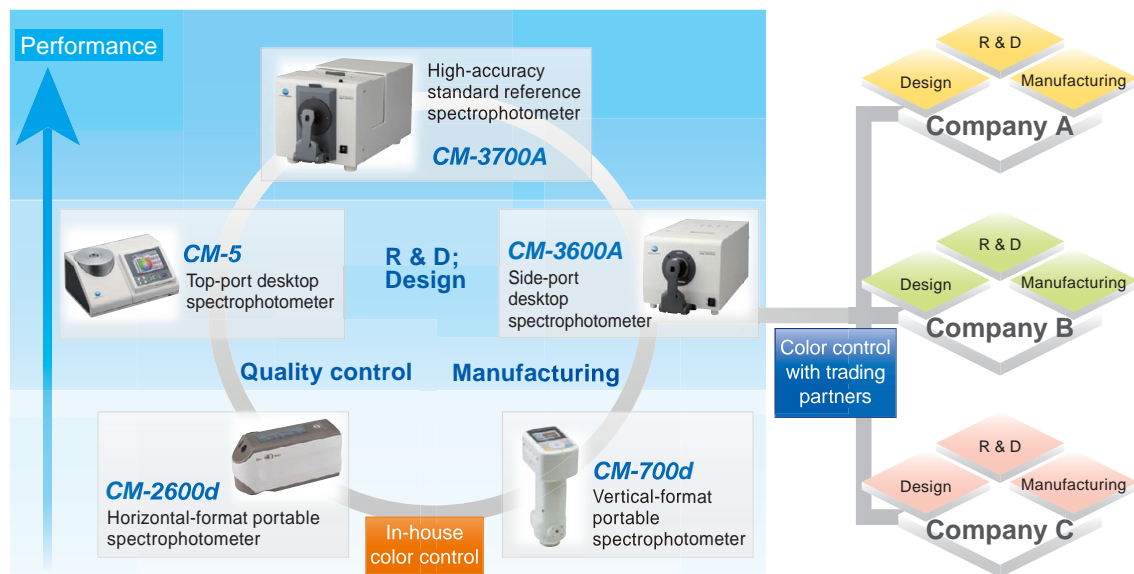

Strict quality assurance system ensures reliability and peace of mind

Konica Minolta's color-measuring instruments are traceable to national standards for wavelength accuracy and white calibration for strict accuracy control. Konica Minolta has also received ISO 9001 and ISO 14001 certification for its integrated quality control system from product development through manufacturing and after-sales service.

Comprehensive support system

Konica Minolta has service facilities worldwide to perform quick inspection, calibration, and repair and ensure that your instruments always provide their best performance.

Measurement functions

Number for unlimited sample length (mm)

(n/0° viewing angle) geometry for measurements of sheet samples such as cells containing liquid samples

Additional Features of CM-3700d

Long sample holder arm enables measurement at center of A4-size sample.



Sample holder arm stays open when opened fully for easy positioning of thick samples.




Frame around power switch prevents switching power off by mistake.



USB communication interface for easy connection and high-speed communication



System Diagram

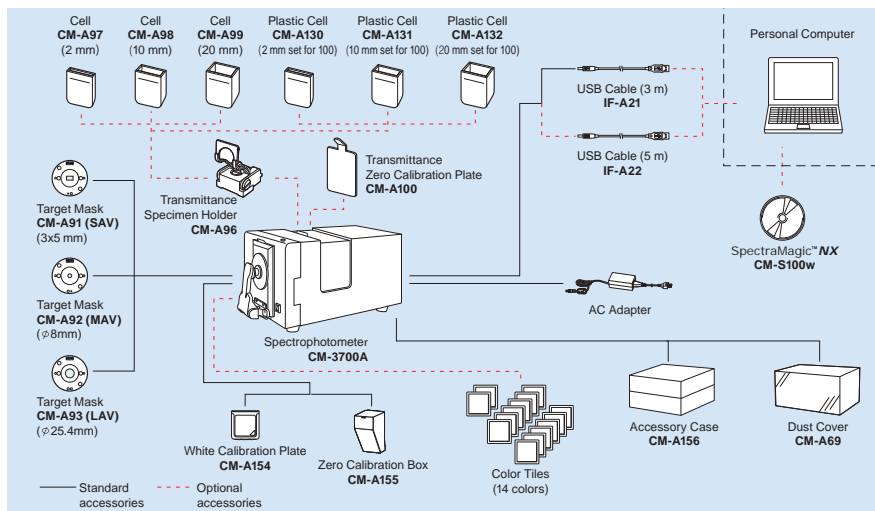

Specifications

Measuring geometry	Reflectance	di:8°, de:8° (diffuse illumination/8° viewing angle) SCI (specular component included)/SCE (specular component excluded) switchable Conforms to CIE No.15, ISO 7724/1, ASTM E 1164, DIN 5033 Teil 7 and JIS Z 8722 condition c standard.
	Transmittance	di:0°, de:0° (diffuse illumination/0° viewing angle) Conforms to CIE No.15, ASTM E 1164, DIN 5033 Teil 7 and JIS Z 8722 condition g standard.
Detector	Silicon photodiode array with flat holographic grating	
Wavelength range	360 to 740 nm	
Wavelength pitch	10 nm	
Half bandwidth	Approx. 14 nm average	
Photometric range	0 to 200%; Resolution: 0.001%	
Light source	Pulsed xenon arc lamp	
Minimum measurement interval	3 seconds	
Illumination/measurement area	Reflectance: Changeable between SAV, MAV, and LAV SAV : 5x7 mm illumination / 3x5 mm measurement MAV : ø11 mm illumination / ø8 mm measurement LAV : ø28 mm illumination / ø25.4 mm measurement Transmittance: ø25 mm / Approx. ø20 mm	
Repeatability	When white calibration plate is measured 30 times at 10-sec. intervals after white calibration has been performed: Spectral reflectance: Standard deviation within 0.05% Chromaticity: Standard deviation within ΔE^*_{ab} 0.005 When black tile (BCRA Series II; reflectance: 1%) is measured 30 times at 10-second intervals after white calibration has been performed: Spectral reflectance: 380 to 740 nm: Standard deviation within 0.02% 360 and 370 nm: Standard deviation within 0.04% Chromaticity: Standard deviation within ΔE^*_{ab} 0.05	
Inter-instrument agreement	Mean ΔE^*_{ab} 0.08 (typical) Average for 12 BCRA Series II color tiles. Max ΔE^*_{ab} 0.3 (corresponds to approx. ΔE^*_{CMC} 0.2) for any of 12 BCRA Series II color tiles compared to values measured with Konica Minolta master body.	
UV adjustment	Computer controlled: continuously variable	
Transmittance chamber	Maximum sample thickness: Approx. 50 mm Maximum sample length: Unlimited (no sides when transmittance chamber cover is open) Sample holder (optional) for holding sheet samples or containers of liquid samples can be installed/removed	
Interface	USB 1.1	
Power	AC 100 to 240 V 50/60 Hz 25 VA (using included AC adapter)	
Operation temperature/humidity range (*1)	13 to 33°C, relative humidity 80% or less (at 33°C) with no condensation	
Storage temperature/humidity range	0 to 40°C, relative humidity 80% or less (at 35°C) with no condensation	
Dimensions (W x H x D)	271 x 274 x 500 mm (10-11/16 x 10-3/4 x 19-11/16 in.)	
Weight	18 kg (39.7 lb.)	

*1 Operating temperature/humidity range of products for North America : 13 to 33°C, relative humidity 80% or less (at 31°C) with no condensation

- The specifications and drawings given here are subject to change without prior notice.
- Company names and product names used herein are trademarks or registered trademarks of their respective companies.
- KONICA MINOLTA and the Konica Minolta logo and the symbol mark, and "The essentials of imaging" are registered trademarks or trademarks of KONICA MINOLTA HOLDINGS, INC. SpectraMagic™ is a registered trademark of KONICA MINOLTA SENSING, INC.

KONICA MINOLTA SENSING, INC.
Konica Minolta Sensing Americas, Inc.
Konica Minolta Sensing Europe B.V.

Osaka, Japan
New Jersey, U.S.A.
European Headquarter / BENELUX
German Office
French Office
UK Office
Italian Office
Swiss Office
Nordic Office
Polish Office
SE Sales Division
Beijing Branch
Guangzhou Branch
Chongqing Office
Qingdao Office
Wuhan Office

Konica Minolta (CHINA) Investment Ltd.

Konica Minolta Sensing Singapore Pte Ltd.
KONICA MINOLTA SENSING, INC.

Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA SENSING Worldwide Offices web page :

©2011 KONICA MINOLTA SENSING, INC.

Optional accessories


Transmittance Specimen Holder CM-A96



Transmittance Zero Calibration Plate CM-A100



Glass Cell CM-A97/CM-A98/CM-A99




Color Tiles (14 colors)



SpectraMagic™ NX(Optional)

Supports Windows® XP/Vista/7

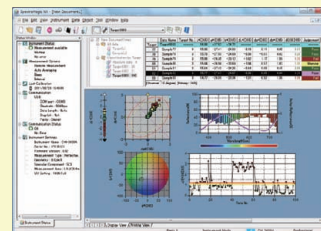

SpectraMagic™ NX enables you to perform comprehensive color inspection and analysis of incoming raw materials, in-process production, and outbound color-critical goods and materials in virtually any industry. With SpectraMagic™ NX you can insert digital images with measured data. Measure samples in any of 8 universally accepted color spaces. Select from 16 illuminants, and up to 40 indices to determine specific color and appearance properties, such as strength, brightness, haze, yellowness, opacity and whiteness. You can even configure up to 8 customized color equations. Reports range from simple Pass/Fail to trend charts, histograms, color plots, and spectral graphs. SpectraMagic™ NX comes with predefined templates, or you can create your own templates. For illustrations and explanations to understanding color and color measurement technology, there is a link to Konica Minolta's well-known and respected "Precise Color Communication", as well as step by step navigation help. Available in 7 languages: English, French, German, Italian, Spanish, Japanese, and Chinese (Simplified/Traditional)

* Windows® is a trademark of Microsoft Corporation in the USA and other countries.

Worldwide sales network



SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the instrument.

- Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.



Certificate No.: LRQ 0960094/A
Registration Date : March 3, 1995



Certificate No.: JQA-E-80027
Registration Date : March 12, 1997

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)
Nieuwegein, Netherlands
München, Germany
Roissy CDG, France
Warrington, United Kingdom
Milan, Italy
Dietikon, Switzerland
Västra Frölunda, Sweden
Wrocław, Poland
Shanghai, China
Beijing, China
Guangdong, China
Chongqing, China
Shandong, China
Hubei, China
Singapore
Seoul, Korea

Fax : 201-785-2482
Fax : +31(0)30 248-1280
Fax : +49(0)89 4357 156 99
Fax : +33(0)1 80 11 10 82
Fax : +44(0)1925 711143
Fax : +39 02 39011.223
Fax : +41(0)43 322-9809
Fax : +46(0)31 474945
Fax : +48(0)71 734 52 10
Fax : +86(0)21-5489 0005
Fax : +86(0)10-8522 1241
Fax : +86(0)20-3826 4223
Fax : +86(0)23-6773 4799
Fax : +86(0)532-8079 1873
Fax : +86(0)27-8544 9991
Fax : +65 6560-9721
Fax : +82(0)2-523-9729

<http://konicaminolta.com/instruments/about/network>

9242-4851-32 BBJAPK① Printed in Japan